

TLN

Department of Forensic Science
Breath Alcohol Section
Instrument Location History
1/1/1990 To 12/15/2014

Instrument Serial Number: 010625

As of 15-Dec-14

Start Date	End Date	Agency Name
15-Dec-14		DFS Central Lab
28-Jul-14	15-Dec-14	Richmond PD
17-Jun-14	28-Jul-14	DFS Central Lab
11-Dec-08	17-Jun-14	Northampton CO SO
15-Aug-08	11-Dec-08	DFS Central Lab

TLN

INTOX EC/IR II **Quality Assurance Worksheet**

Instrument Serial Number **010625** Worksheet Start Date **12/15/2014**

Location **Richmond PD 4th Precinct**

Address **2219 Chamberlayne Ave Richmond VA 23222**

DFS Technician **Timmy Neece, Jr** License No. **25387**

☐ Laboratory ☒ On-Site

Site Specification: No detrimental environmental conditions exist. ☒

Instrument Barometer (mm HG) **758** Reference Barometer (mm HG) **759**

Reference Barometer(RB)Serial # **009111** RB Calibration Due **5/19/2015**

Measurement Assurance Check

Standard (sea level)	PA Target	minimum	maximum	Sample 1	0.301
0.300	0.299	0.290	0.307	Sample 2	0.301
Precision		sample min	sample max	Sample 3	0.300
0.001		0.300	0.301		

Standard (sea level)	PA Target	minimum	maximum	Sample 1	0.100
0.100	0.100	0.097	0.103	Sample 2	0.099
Precision		sample min	sample max	Sample 3	0.099
0.001		0.099	0.100		


Dry gas standard Lot No. (with tank no.) **AG332301-12**

☐ Replaced dry gas standard (+O-ring)

☐ Installed at Location

☒ Removed to DFS-Central

Supplies
Mouthpieces
Certificates of Analysis
Operator Worksheet
Other:



Notes:

Instrument Serial Number

010625

Certification Date

☐ Calibrated☐ Certified☒ Measurement Assurance Check☒ Instrument Test☐ Troubleshooting/Maintenance Worksheet Completed

(Successful completion denotes satisfactory condition of the item.)

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.250		0.000	0.000	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.150		0.000	0.000	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	


Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.080		-0.003	0.003	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.020		-0.003	0.003	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

All measurements are in g/210L

Estimation of Uncertainty of Measurement and traceability records are located within the Breath Alcohol Section


DFS Technician



Date

12/15/14

Issuing Analyst

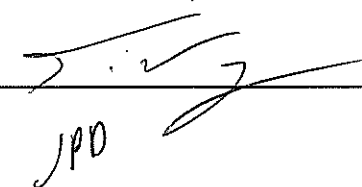
JPD

Date

12/15/14

TLW




COMMONWEALTH OF VIRGINIA
DEPARTMENT OF FORENSIC SCIENCE

CERTIFICATE OF BLOOD ALCOHOL ANALYSIS
AS DETERMINED BY A CHEMICAL TEST OF THE ACCUSED'S BREATH

NAME OF ACCUSED INSTRUMENT, TEST,	NAME OF COURT DFS
--	--------------------------

BREATH ANALYSIS

SAMPLE EXAMINED AND TEST CONDUCTED BY NEECE, JR., TIMMY, L		AGENCY DFS Central Lab
DFS LICENSE NUMBER 25387	LICENSE EXPIRES 10/01/2016	DATE TEST CONDUCTED 12/15/2014
TEST EQUIPMENT NUMBER 010625		

RESULTS: TIME SAMPLE TAKEN 13:43 EST

SAMPLE'S ALCOHOL CONTENT 0.00 GRAMS PER 210 LITERS OF BREATH

ATTEST:

I CERTIFY THAT THE ABOVE IS AN ACCURATE RECORD OF THE TEST CONDUCTED; THAT THE TEST WAS CONDUCTED WITH THE TYPE OF EQUIPMENT AND IN ACCORDANCE WITH THE METHODS APPROVED BY THE DEPARTMENT OF FORENSIC SCIENCE; THAT THE TEST WAS CONDUCTED IN ACCORDANCE WITH THE DEPARTMENT'S SPECIFICATIONS; THAT PRIOR TO ADMINISTRATION OF THE TEST THE ACCUSED WAS ADVISED OF HIS RIGHT TO OBSERVE THE PROCESS AND SEE THE BLOOD ALCOHOL READING ON THE EQUIPMENT USED TO PERFORM THE BREATH TEST, AND THAT I POSSESS A VALID LICENSE TO CONDUCT SUCH TEST, GIVEN UNDER MY HAND THIS _____ DAY OF _____, 20 _____.

BREATH TEST OPERATOR

☐ I HAVE RECEIVED A COPY OF THIS CERTIFICATE OF ANALYSIS _____ SUBJECT'S SIGNATURE

☐ SUBJECT REFUSED TO SIGN FOR COPY OF CERTIFICATE OF ANALYSIS _____ OPERATOR'S SIGNATURE



IntoxNet MIS Report

Report Generated 15 Dec 2014 at 14:15

mmB
TLN

Test Results

Instrument Serial Number 010625

Test # 000553 Subject Test

Test Location 1 Department of
Test Date 15 Dec 2014

Test Location 2 Forensic Science
Test Time 13:37
Remote/Local Local

Test Location 3
System Check Passed

Operator's Last Name NEECE, JR.
Agency DFS Central Lab

Operator's First Name TIMMY

Operator's Middle Initial L

Card Serial Number 125387

License Number 25387

Effective Date 10/01/2014

Expiration Date 10/01/2016

Subject's Last Name INSTRUMENT

Subject's First Name TEST

Subject's Middle Initial

Subject's Date of Birth 00/00/0000

Subject's Sex Male

Driver's License Number

Driver's License Expiration 00/00/0000

Driver's License State

Court Name DFS

End Date 15 Dec 2014 End Time 13:45

Result Time 13:43

Result Date 15 Dec 2014 Result 0.00

Data Type DIAG

Sample Value Pass

Sample Time 13:37

Data Type BLK

Sample Value 0.000

Sample Time 13:38

Data Type CHK

Sample Value 0.100

Sample Time 13:39

Data Type BLK

Sample Value 0.000

Sample Time 13:40

Data Type SUBJ

Sample Value 0.000

Sample Time 13:41

Data Type BLK

Sample Value 0.000

Sample Time 13:42

Data Type SUBJ

Sample Value 0.000

Sample Time 13:43

Data Type BLK

Sample Value 0.000

Sample Time 13:44

Standard Type Dry Gas Std

Standard Value 0.100

Standard Lot Number AG332301-12

Standard Expiration Date 11/19/2015

Tank Pressure 389

Barometric Pressure 758 mmHg

Blow Sample Number 1 Blow Duration 3.13 sec

Blow Volume 1926 cc End-of-Blow Time 13:41

Blow Sample Number 2 Blow Duration 3.17 sec

Blow Volume 1826 cc End-of-Blow Time 13:43

Tamper Evident Stamp a20e1a66

Test Status Code 0

Test Status Success

TLN

Intox EC/IR-11: Accuracy Check

Department of Forensic Science

Serial Number: 010625 Test Number: 554

Test Date: 12/15/2014 Test Time: 13:48 EST

Dry Gas Target: 0.100

Lot Number: AG332301-12 Exp Date: 11/19/2015

Tank Pressure: 389 psi Barometric Pressure: 758 mmHg

System Check: *Passed*

Test	g/210L	Time
BLK	0.000	13:48
CHK	0.100	13:49
BLK	0.000	13:51
CHK	0.099	13:51
BLK	0.000	13:53
CHK	0.099	13:54

Test Status: *Success*

Calibration CRC: BB41C735

TLN

Intox EC/IR-II: Accuracy Check

Department of Forensic Science

Serial Number: 010625 Test Number: 555

Test Date: 12/15/2014 Test Time: 13:57 EST

Dry Gas Target: 0.299

Lot Number: AG428003-03 Exp Date: 10/07/2016

Tank Pressure: 340 psi Barometric Pressure: 758 mmHg

System Check: Passed

Test	g/210L	Time
BLK	0.000	13:59
CHK	0.301	13:59
BLK	0.000	14:01
CHK	0.301	14:02
BLK	0.000	14:04
CHK	0.300	14:05

Test Status: Success

Calibration CRC: BB41C735